


UT303D QA检验测试报告

使用仪器: FLUKE黑体

环境温湿度: 25.4℃ / 65.2%

功能	量程	输入		准确度	最大允许误差		读数范围			测试值	测试结果	
温度及激光	℃	-32.0	℃	1.8%	±	-1.8	-33.4	~	-30.6	℃	-33.1	合格
	℃	-18.0	℃	1.8%	±	-1.8	-19.4	~	-16.6	℃	-19.2	合格
	°F	32.0	°F	1.8%	±	4.0	28.8	~	35.2	°F	33.2	合格
	℃	20.0	℃	1.8%	±	1.8	18.6	~	21.4	℃	20.3	合格
	℃	75.0	℃	1.8%	±	1.8	73.6	~	76.4	℃	35.1	合格
	℃	75.0	℃	10.0%	±	7.5	69.0	~	81.0	℃	73.6	合格
	°F	302.0	°F	1.8%	±	5.4	297.7	~	306.3	°F	302.1	合格
	℃	350.0	℃	1.8%	±	6.3	345.0	~	355.0	℃	349.9	合格
	℃	545.0	℃	1.8%	±	9.8	537.2	~	552.8	℃	546.3	合格
	℃	745.0	℃	1.8%	±	13.4	734.3	~	755.7	℃	745.6	合格
	℃	945.0	℃	1.8%	±	17.0	931.4	~	958.6	℃	948.0	合格
	℃	1020.0	℃	1.8%	±	18.4	1005.3	~	1034.7	℃	1019.3	合格
	℃	1220.0	℃	1.8%	±	22.0	1202.4	~	1237.6	℃	1217.5	合格
℃	1520.0	℃	1.8%	±	27.4	1498.1	~	1541.9	℃	1522.7	合格	

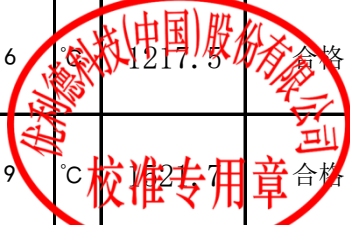

检测员: 张琼

审核员: 郭桂余